


SYMBOL	REVISION REQUIRED	DATE	AUTH.

Notes:

1. All dimensions in millimeters.
2. Normal tolerances ± 0.5 mm
3. SENSITIVITY: 30 minutes/ 2mm
Tolerance on sensitivity is ± 15 %.

MATERIAL: ACRYLIC
FLUID: CLEAR

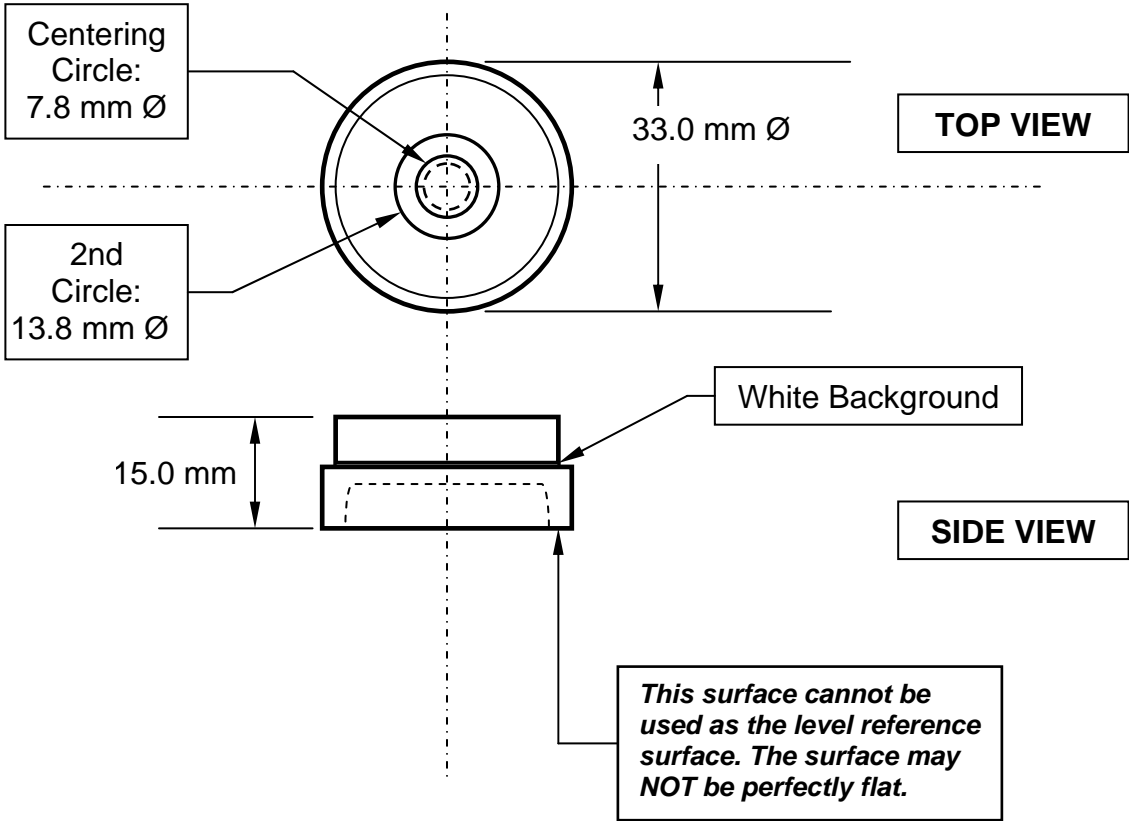

GEIER & BLUHM, INC.
594 River Street
Troy, NY 12180 USA

DRAWN BY: DAVID OSTER

DATE: February 24, 2009

Scale: NONE

DRAWING NUMBER

VIAL, CIRCULAR LEVEL

1-20530