

SYMBOL	REVISION REQUIRED	DATE	AUTH.
A	Redrawn	6/18/1982	R.L.O.
B	Overall Height was .328"	3/08/1989	V.J.C.
C	Redrawn, revised notes, P/N was 2-8010	11/17/2004	D.B.O.


**Notes:**

1. All dimensions are in inches.
2. SENSITIVITY: 45 minutes/ 0.1" movement of the bubble. Tolerance on sensitivity is  $\pm 10\%$ .
3. Part or all of the finish maybe removed from Surface "X" during calibration.

**MATERIAL:** Housing: Brass  
Vial: Glass

**FLUID:** Clear Mineral Spirits

**FINISH on Housing:** Chrome-Plate

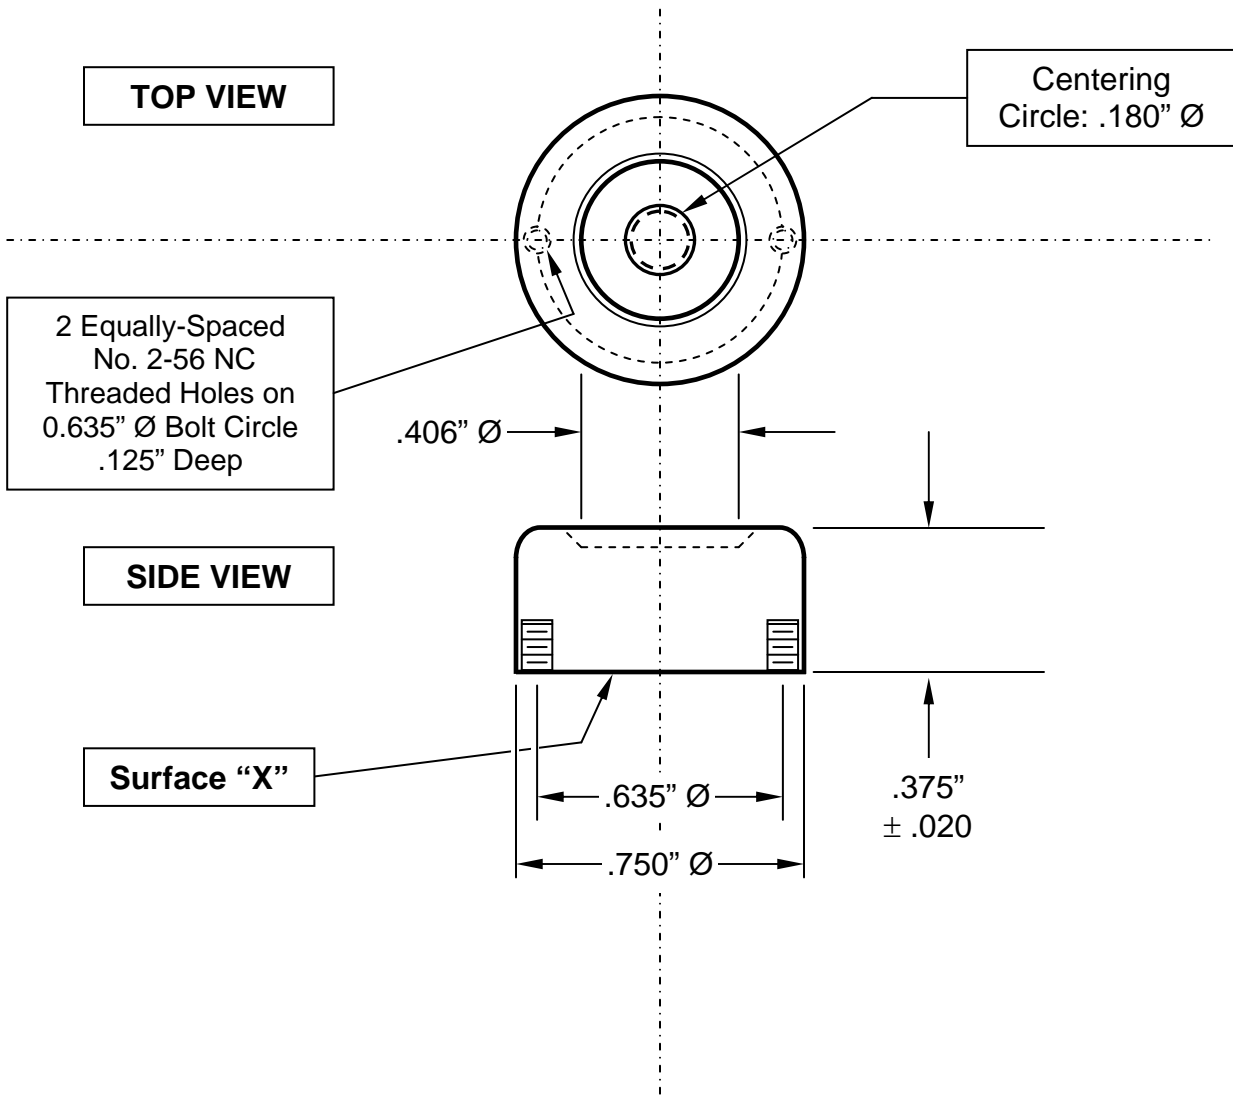

<b>Tolerances: (except as noted)</b>	<b>Decimal <math>\pm .010</math>"</b>	<b>Fractional <math>\pm 1/64</math>"</b>	<b>Angular <math>\pm 1^\circ</math></b>
--------------------------------------	---------------------------------------	--	---

<b>GEIER &amp; BLUHM, INC.</b> 594 River Street Troy, NY 12180 USA	DRAWN BY: DAVID OSTER	DATE: November 17, 2004
	Scale: NONE	DRAWING NUMBER
	<b>MOUNTED CIRCULAR LEVEL</b>	<b>2-08010</b>