


SYMBOL	REVISION REQUIRED	DATE	AUTH.
A	Redrawn, revised notes	5/28/2004	D.B.O.

**Notes:**

1. All Dimensions in inches except as noted
2. SENSITIVITY: 1.0 minutes/Division (2mm)  
Tolerance on sensitivity is +/- 15%
3. Part or all of the finish maybe removed from Surface "X" during calibration
4. When the bubble is centered in the 8 mm centering circle, the Level is level within  $\pm .2$  minutes.

**MATERIAL:** Housing: Brass  
Vial: Glass  
**FINISH on Housing:** Chrome  
**FLUID:** Methanol  
**COLOR of FLUID:** Clear

**TOLERANCES:**  
Decimal: +/- .010"  
Fractional:  $\pm 1/64$ "  
Angular:  $\pm 1/2^\circ$

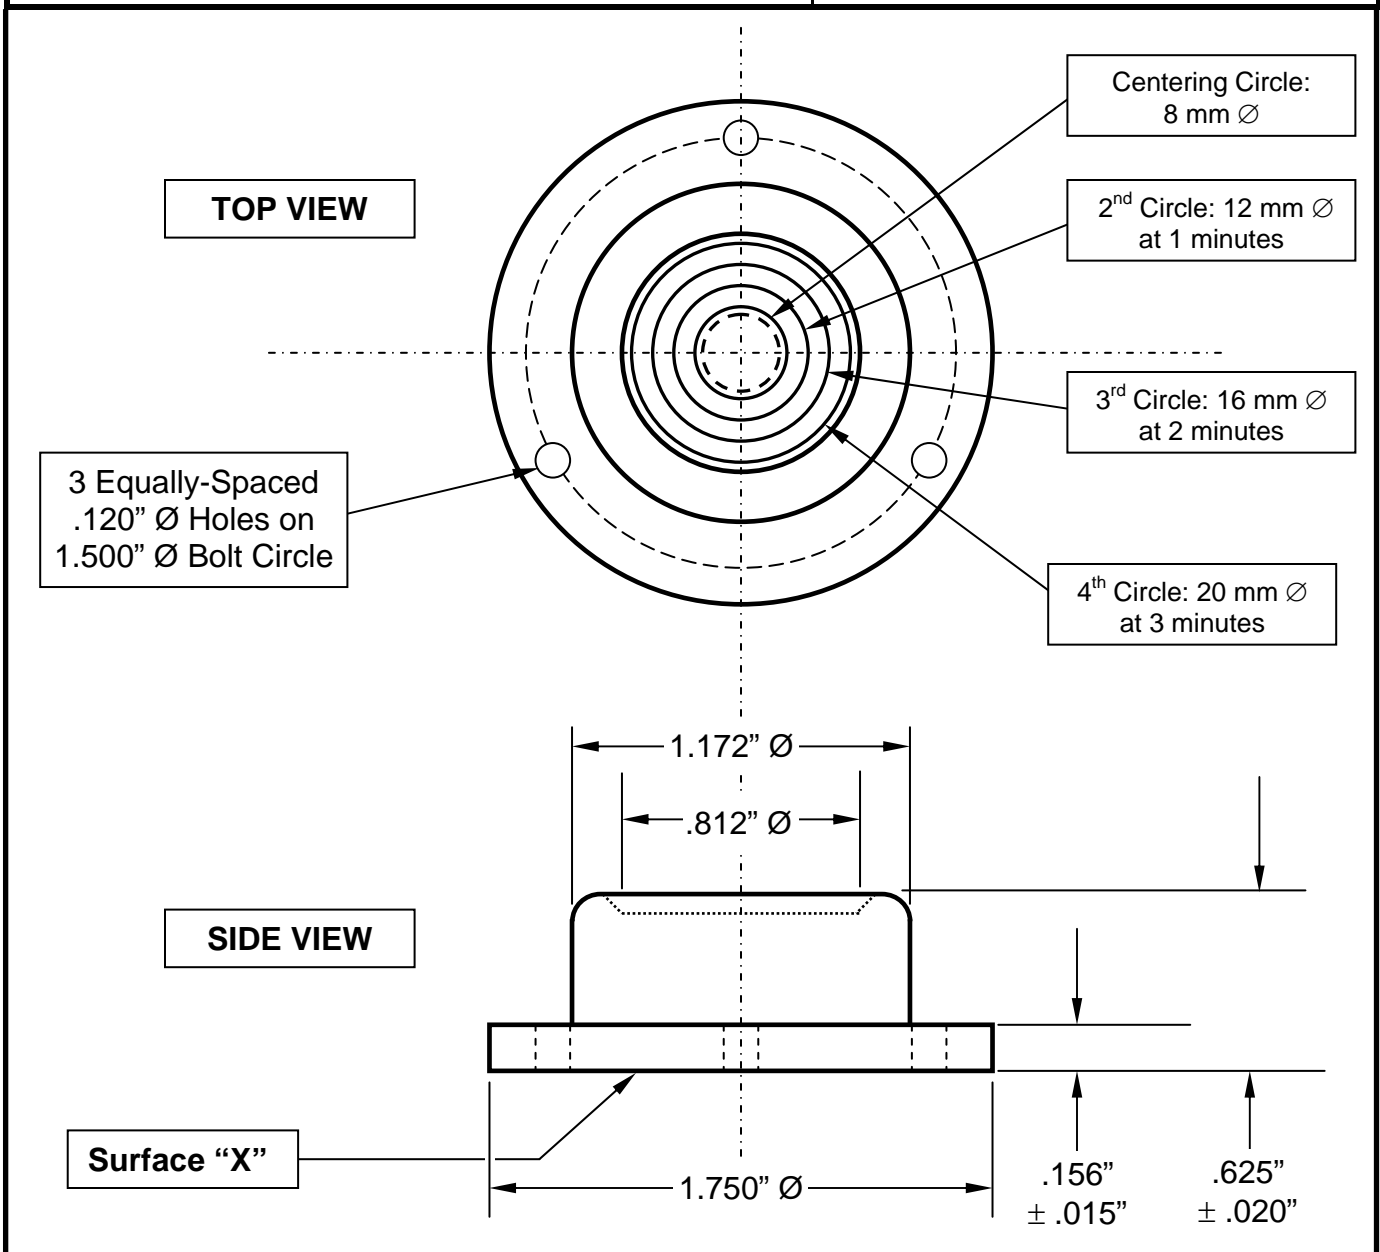

<b>GEIER &amp; BLUHM, INC.</b> 594 River Street Troy, NY 12180 USA	DRAWN BY: DAVID OSTER	DATE: July 21, 2000
	Scale: NONE	<b>DRAWING NUMBER</b>
	<b>MOUNTED CIRCULAR LEVEL</b>	<b>2-16046</b>