


SYMBOL	REVISION REQUIRED	DATE	AUTH.

Notes:

1. All dimensions are in millimeters
2. Normal tolerances +/- 0.5 mm
3. SENSITIVITY: 30 minutes/ 2mm
Tolerance on sensitivity is +/- 10 Minutes.

MATERIAL: ACRYLIC
FLUID: GREEN-YELLOW

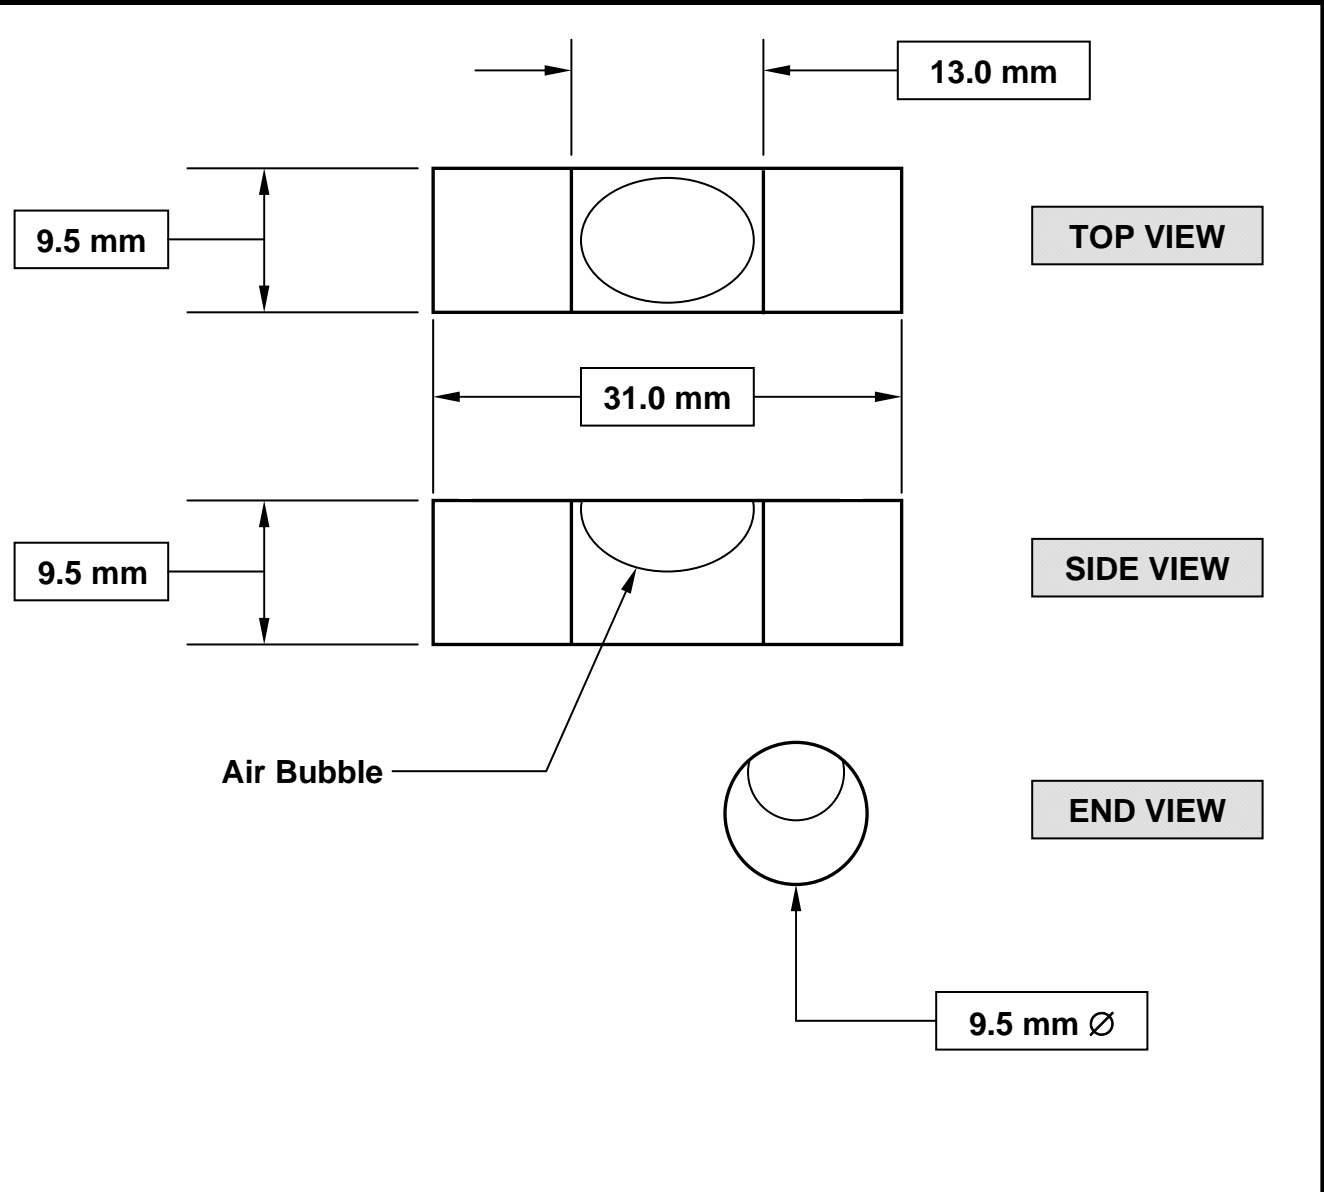

GEIER & BLUHM
Division of HJM Precision, Inc.
594 River Street
Troy, NY 12180 USA

DRAWN BY: DAVID OSTER
Scale: NONE

DATE: January 12, 2012
DRAWING NUMBER

**TUBULAR LEVEL
VIAL**

3-1519