


SENSITIVITY 60 Seconds for each Division Sensitivity Tolerance: ± 6 seconds (Division Spacing is 2 mm)	SYMBOL	REVISION RECORD	DATE	AUTH.
	A	Redrawn and Added Notes	1/07/1999	D.B.O.
	B	Redrawn	6/7/2004	D.B.O.
	C	Redrawn	4/8/2008	D.B.O.

NOTES:

- (1) All Dimensions are in Inches.
- (2) Bubble Length: same as shown at 70° F to 75° F
- (3) Protective Finish on Housing: Black Lacquer Paint
- (4) Surface "A" has a relief approximately 1/64" deep.
- (5) Level is calibrated to within 30 seconds with respect to Surface A and the horizontal plane.

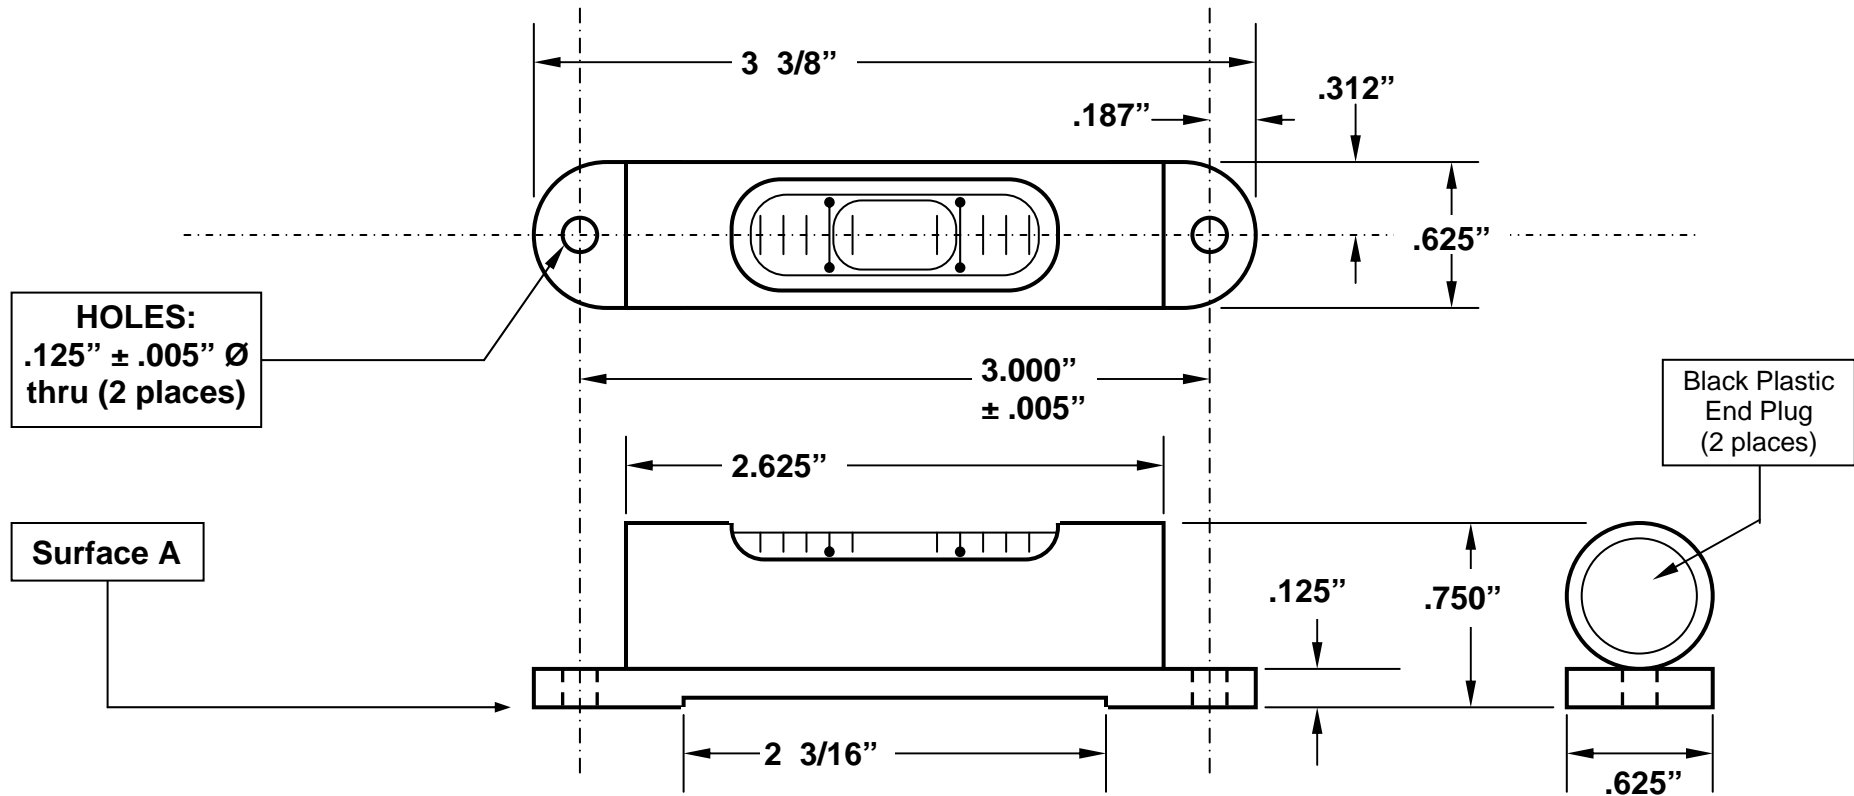

GEIER & BLUHM, INC. 594 River Street Troy, New York 12180 U.S.A. TEL: 518-272-6951 FAX: 518-272-0533	TOLERANCES: (Except as noted) Decimal: $\pm .010$ " Fractional: $\pm 1/64$ " Angular : $\pm 1/2$ degree FLUID: Clear Methanol	MATERIAL: Vial: Glass Housing: Brass SCALE: NONE	DRAWN BY: DAVID OSTER	DATE: July 25, 1975
			PLATE LEVEL	